



IMAGE IN CARDIOLOGY

Impact of mechanical mitral prosthesis on transcatheter aortic valve implantation procedure

Impacto da presença de uma prótese mitral mecânica na implantação de uma válvula aórtica percutânea

Joana Certo Pereira^{a,*}, Ana Rita Bello^a, Francisco Albuquerque^a, João Abecasis^{a,b}, Pedro de Araújo Gonçalves^{a,c,d}

^a Department of Cardiology, Hospital de Santa Cruz, Carnaxide, Lisbon, Portugal

^b Department of Cardiology, Hospital dos Lusíadas, Lisbon, Portugal

^c Department of Cardiology, Hospital da Luz, Lisbon, Portugal

^d NOVA Medical School, Lisbon, Portugal

Received 20 March 2025; accepted 19 August 2025

Case presentation

An 82-year-old woman, with a previous mechanical mitral valve (MMV) replacement for rheumatic mitral stenosis, presented with symptomatic severe aortic stenosis. The transthoracic echocardiogram (TTE) showed an aortic valve mean gradient of 57 mmHg, aortic valve area of 0.5 cm² and left ventricular ejection fraction (LVEF) of 48%. The patient had a high operative risk (Euroscore II: 24%), suitable femoral access, an aortic valve calcium score of 2700 Agatston units, and a mean annulus diameter of 21.5 mm. The heart team opted for replacement of the damaged valve. The new valve was then placed inside the diseased valve, and transcatheter aortic valve replacement (TAVI) was performed using a self-expanding, recapturable Corevalve Evolut Pro 26 mm

On the first attempt, the TAVI was placed in high position to avoid interference with MMV, but this attempt was aborted due to several “pop out” events. The TAVI was then repositioned lower and in this final implantation position there was underexpansion of the proximal strut, but no interference with MMV or with the TAVI leaflets. Post-dilatation was not performed due to potential risk of disruption of the MMV.

The post-procedure TTE showed a moderate paravalvular leak, with normal transvalvular gradients across the aortic and mitral valves (mean gradients of 9 mmHg and 4 mmHg, respectively).

A post-procedural cardiac computed tomography to assess prosthesis morphology and the residual regurgitation mechanism was performed¹ (Panel 1).

At one-year follow-up, the patient was stable, with no congestion, no hemolysis, improved LVEF (>55%), a mild paravalvular leak, and normal transvalvular gradients across both the aortic and mitral valves (mean gradients of 7 mmHg and 3 mmHg, respectively).

* Corresponding author.

E-mail address: joanacerto@gmail.com (J. Certo Pereira).

<https://doi.org/10.1016/j.repc.2025.08.005>

0870-2551/© 2025 Sociedade Portuguesa de Cardiologia. Published by Elsevier España, S.L.U. This is an open access article under the CC BY-NC-ND license (<http://creativecommons.org/licenses/by-nc-nd/4.0/>).

Please cite this article as: J. Certo Pereira, A.R. Bello, F. Albuquerque et al., Impact of mechanical mitral prosthesis on transcatheter aortic valve implantation procedure, Revista Portuguesa de Cardiologia, <https://doi.org/10.1016/j.repc.2025.08.005>

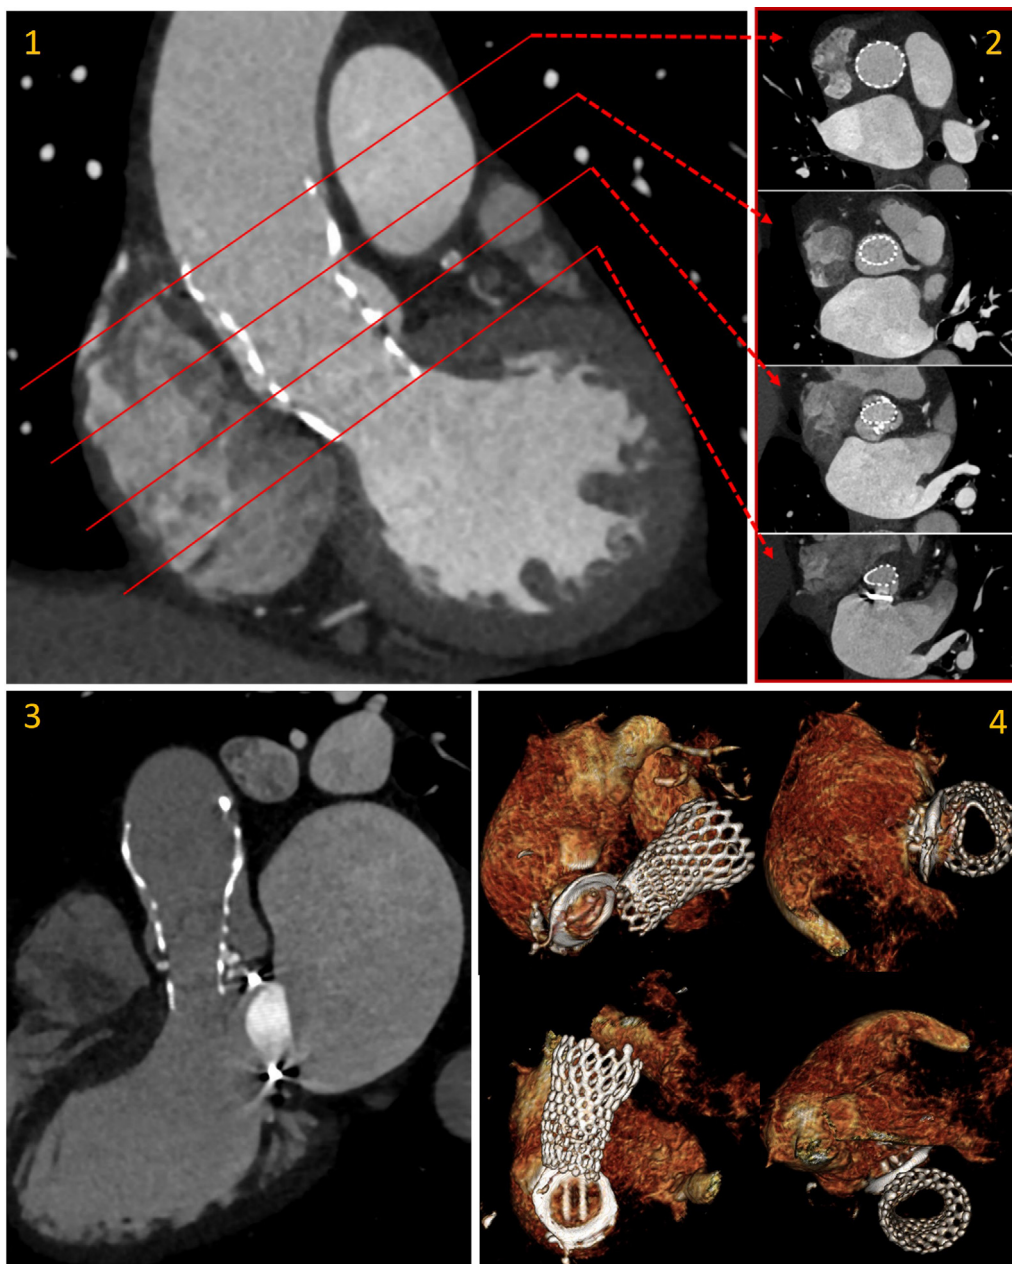


Figure 1 Post-procedural cardiac CT to access prosthesis morphology: modified coronal plane (1), short-axis (2), long-axis 3-chamber view (3) and volume rendering depicting the relation of TAVI prosthesis with the MMV with the restriction in expansion (elliptical shape) in the distal struts (4). This deformation is below the plane of the valve (CoraValve has a supraannular design).

Transcatheter aortic valve replacement in MMV patients requires careful device selection and precise positioning due to the balance between avoiding MMV interference with low implantation and minimizing embolization risk from high positioning in mildly calcified valves.² For this patient we considered this position the best possible result (Figure 1).

her medical case in a peer-reviewed medical journal. The authors of this article (J.C.P. and A.R.B.) obtained written informed consent from the patient, in accordance with COPE guidelines. The authors declare that the figures in the article do not enable patient identification. Dates were omitted to comply with confidentiality. This case report was exempt from ethics board approval.

Ethical approval

We obtained informed consent from the patient to publish this case report, as well as any images associated with the case. The patient verbally consented to the publication of

Funding

None declared.

Conflict of interest

None declared.

Appendix A. Supplementary data

Supplementary material associated with this article can be found in the online version at <https://doi.org/10.1016/j.repc.2025.08.005>.

References

1. Soschynski M, Capilli F, Ruile P, et al. Post-TAVI follow-up with MDCT of the valve prosthesis: technical application, regular findings and typical local post-interventional complications. *Rofo*. 2018;190:521–30.
2. Chmielak Z, Dąbrowski M, Tyczyński P, et al. Transcatheter aortic valve replacement in patients with previous mitral valve replacement. A systematic study. *Postepy Kardiol Interwencyjnej*. 2020;16:177–83.